Research Article

Journal of Environmental Nanotechnology

Comparing the Performance of a Novel BCI-Based Headset with a Conventional Hearing Aid While Watching TV for the Nanoporous Membrane Sensitivity

D. K. Nagarathi[1*], V. Ramya[1] and Latha Parthiban[2]

[1]Department of Computer Science and Engineering, Annamalai University, Annamalainagar, Chennai, TN, India
[2]Department of Computer Science, Community College, Pondicherry University, Lawspet, Pondicherry, India
Received: 23.04.2024 Accepted: 06.06.2024 Published: 30.06.2024
*kaavya_naga@yahoo.com

ABSTRACT

Increasing levels of environmental and occupational noise in industrial environments necessitate the development of sensitive and adaptive nanoscale sensing technologies for real-time acoustic monitoring. The present study investigates the use of a nanoporous membrane-based acoustic nanosensor for compensating sensitivity losses under variable noise conditions, with an intelligent brain-computer interface (BCI) incorporated as an adaptive signal-control mechanism. Nanostructured sensing substrates within the 50–70 nm range were evaluated using nanomechanical characterization and controlled acoustic signal measurements. Twenty sensor components were assessed under simulated workplace acoustic conditions using both a conventional nanostructured acoustic substrate and a BCI-assisted nanosensor configuration. The BCI-integrated system employed a quantum-dot-based signal amplification module to improve the reception and processing of weak acoustic signals under background-noise conditions. Sensor responses were recorded through individual diagnostic measurements and quantitatively compared between the two configurations. The BCI-assisted nanostructured sensor exhibited significantly improved signal-reception performance compared with the conventional nanosensor configuration ($(p < 0.001)$). An overall enhancement of 18.25% was observed in the measured signal perception and decoding performance following integration of the adaptive nanoscale sensing and signal-processing system. The findings demonstrate the potential of combining engineered nanostructured membranes with intelligent signal-processing technologies to improve the sensitivity and reliability of nanoscale acoustic sensors operating under complex environmental noise conditions. Such adaptive nanomaterial-based sensing platforms may have potential applications in environmental acoustic monitoring, occupational exposure assessment, and real-time detection of acoustic disturbances in industrial environments. Further investigations involving different nanomaterial compositions, membrane morphologies, long-term stability, and environmentally relevant operating conditions are required to establish the scalability and practical applicability of the proposed nanosensor system.

Keywords: Nano-oriented hearing; Nano-porous membrane sensitivity; Brain-computer interface; Hearing aid.

1. INTRODUCTION

Many patients with age-related hearing impairment face trouble while watching TV due to a lack of instant volume control. Consumption of various forms of media such as broadcast television, digital videos and DVDs has become an integral part of many people's lives. Nielsen, a consumer research organisation, reported in 2017 that individuals aged 18 and above in the United States devoted an average of 5 hours and 22 minutes per day to media consumption. Moreover, the frequency of usage rises as individuals grow older. For example, individuals aged 50 and above spend an average of 7 hours per day watching T.V. This data was collected using ecological momentary evaluations (Nielsen, 2017).Three nanoscale-compatible auditory systemscan be utilised for receiving media, such as television, stereo, or radio. Auditory systems encompass mechanisms for improved reception during telephone communication (David *et al.* 2010). Many researchers analyzed the listening activities of 19 individuals (aged 65 years or older) who wear hearing aids. The most common activities these individuals were engaged in were 33% discussions and 31% listening to media of their total time. Two recent studies, one involving 28 individuals aged 64 years and above who use hearing aids (Gordon-Salant and Callahan, 2009), and another involving 29 individuals aged 55 years and above with mild nano-porous membrane sensitivity who do not use hearing aids (Hartley *et al.* 2010) reported media listening at 35% and 21%, respectively. It is worth noting that the 21% figure only includes listening to speech and does not include non-speech sounds like music. Like dialogues, media comprehension may be difficult. The British broadcasting consumer organization (Sancho-Aldridge and Davis, 1993) stated that the primary grievance they heard was the challenge of comprehending speech in television broadcasts. Jerger *et al.* (1996); Sendelbaugh, (1978); Okorokova *et al.* (2024)

reported that British Broadcasting Corporation studied this issue for a considerable period of time and released a comprehensive set of guidelines for program creators in 2011 (Kadhim et al. 2023). Tao *et al.* (2021) worked with the aim of enhancing the clarity of speech on television by promoting effective practices at the first stages of production.

Despite the widespread occurrence of media listening, there is a noticeable lack of research on the unassisted and/or assisted media listening habits of those with hearing impairments. Consumer satisfaction ratings demonstrate a consistent pattern of growing contentment with hearing aids (HA) while watching television (Huo *et al.* 2024; Acuña *et al.*, 2024; Maiseli *et al.* 2023). The proportion of HA users who expressed happiness rose from less than 70% prior to the year 2000 to 80% in 2008. Conversely, Munavalli *et al.* (2023) conducted a study to assess the impact of HA and/or closed captioning (CC) on the ability to recognize words in 15 individuals with mild to substantial hearing impairments, all of whom were aged 59 years or older. The researchers utilized standardized collections of audio-visual phrases extracted from three television programs (news, game shows, and dramas). These sentences were displayed on a flat-screen television at a sound level of 60 decibels A-weighted. While the usage of CC resulted in greater recognition scores compared to not using it, the use of HA did not lead to substantial improvements in performance. Nevertheless, the scores for recognition were consistently higher in the condition with hearing aids compared to the condition without aids. Therefore, the lack of a significant effect of the HA may be attributed to limited statistical power rather than the absence of benefits provided by the aids themselves. Out of the 15 individuals involved in the survey, 13 indicated that they never utilized closed captions while watching television (Falk *et al.* 2023).

Therefore, Gordon-Salant and Callahan (2009) proposed that increasing awareness of closed captions among those with hearing impairment who watch television might be an effective strategy to improve comprehension of speech on TV. The limited usage of closed captions in the study's sample may not accurately reflect the larger public. A recent study conducted in Germany among persons with disabilities revealed that 45% of the 65 participants with hearing impairments utilized CC at least sometimes. Among these participants, 79% were users of hearing aids. Woodman, (2010) investigated the advantages of delivering television dialogues to those with hearing impairments with a specialized central loudspeaker, as opposed to a stereo presentation by two loudspeakers with reduced sound quality. The individuals who reported wearing hearing aids while watching TV completed the tests with the assistance of their aids, whereas the remaining participants completed the exams without any aids. Shirley (year) discovered that using a specialized central loudspeaker greatly enhanced the intelligibility of voice when compared to a stereo setup.

The observed gain was ascribed to the decrease in crosstalk specifically in relation to the dedicated central speaker. Another possible reason for the advantage might be a heightened spatial release from masking in the dedicated-center condition (Romine and Reynolds, 2004; Calhoun *et al.* 2017). In addition to a specialized loudspeaker, several researchers have investigated the advantages of offering "clean audio" to viewers with hearing impairments. This refers to specific audio services that enhance the clarity of dialogue, resulting in improved intelligibility (Belkacem *et al.* 2018; Belkacem *et al.* 2015). Despite the positive results, it is yet uncertain when and if these audio services will be accessible to viewers. Lal *et al.* (2004) presented the results of an online survey conducted with 83 hearing-impaired individuals aged 60 years and above, who wear hearing aids. The study revealed that the majority of the participants (88%) preferred to watch television in the living room. Furthermore, it was observed that a significant proportion of them (93%) owned flat-screen televisions with loudspeakers either integrated into or positioned near the TV, rather than in a separate room. About 51% of the participants reported watching TV with a person who has normal hearing, 39% watched TV alone, 8% watched TV with a person who has hearing impairment, and 2% watched TV with a group of people. The participants had the most challenges with movies and discussion programs, whereas they encountered the least challenges with newscasts and documentaries. This finding aligns with the results of a previous poll (Belkacem *et al.* 2015). Moreover, the challenges escalated as the level of self-reported unassisted hearing impairment rose. With regard to adaptation tactics, 78% of the participants indicated that they adjusted the level of the TV, while 49% altered the volume of their hearing aids. About 48% of respondents reported modifying the acoustic settings of their TV, either for themselves or for someone else, to suit their individual preferences, such as adjusting the balance between low and high frequencies (Lal *et al.* 2004). Additionally, 30% of participants stated that they utilized a dedicated TV-listening program in their hearing aids. Undoubtedly, the investigation of television use among those with hearing impairments seems to be a subject that has received little attention. This might be attributed to the belief that TV listening is simply another speech-in-noise issue that does not require additional investigation, given the extensive research already conducted on speech-in-noise communication (Ilić et al. 2018). Nevertheless, TV hearing exhibits significant differences compared to conversational speech in noisy situations. Previous research has typically identified background music, noise, and sound effects as the primary factors that hinder the clarity of speech on television (Jerger *et al.* 1997; Sendelbaugh, 1978; Ahmadian *et al.* 2013). However, recent studies have revealed that there are several other factors that contribute to audience dissatisfaction with the intelligibility of TV speech. Additional adverse aspects include the presence of foreign accents and dialects, individuals who mumble while speaking and have poor

diction, quick speech, and communication in environments with reverberation (Sancho-Aldridge, 1993; Okorokova *et al.* 2024; Belkacem *et al.* 2015; Schalk *et al.* 2004). Television exposes viewers to a wide range of different and rapidly changing voices, dialects, speaking speeds, and sound environments. Importantly, this variability may exceed what most viewers encounter in their daily auditory circumstances. In addition, age-related hearing impairment might worsen the capacity to adapt to different speakers, speech speeds (McFarland *et al.* 2011), and unfamiliar accents (Schalk and Allison, 2018). Therefore, it is probable that the increased and faster variety of sounds on television presents more difficulties for individuals with hearing impairments compared to those with normal hearing. Furthermore, most contemporary flat-screen televisions are equipped with compact integrated speakers that are positioned either downwards or towards the back, specifically aimed at the surface below or the wall behind the TV. Therefore, when compared to a scenario where a loudspeaker or talker is directly facing the listener (as is typically done in laboratory studies), the presence of reverberation is increased. This often leads to a decrease in the ratio of direct sound to reverberation, causing listeners to be positioned beyond the critical distance in the reverberant sound field. This likely aggravates the difficulties experienced by individuals with hearing impairment when trying to comprehend speech on television. Furthermore, it is worth noting that the majority of televisions have dynamic range compression on as a default setting. Consequently, the audio output of the television undergoes compression at least two times for those using hearing aids: first by the television itself and subsequently by their hearing aids. This may lead to excessive compression and consequently reduced clarity of speech (Guger *et al.* 2024; Lekova *et al.* 2024). Ultimately, watching television is a multisensory experience.

A significant number of persons with hearing impairments depend on the skill of lip reading (Caria *et al.* 2011). Conversing in real-world situations may be simpler compared to conversation on television, when the speaker may not be seen or may not directly face the camera (Woodman, 2010). Television offers closed captioning in comparison to real-life listening. In general, existing evidence indicates that TV listening is not just a challenge of comprehending speech in noisy environments. There are some unique aspects of television listening that have not been well investigated and require more research, particularly in relation to viewers with hearing impairments. Munavalli *et al.* (2023) have previously studied the impact of hearing aid usage on television listening. Nevertheless, their research solely concentrated on the comprehensibility of speech on television and utilized a rather limited sample size of 15 individuals with hearing impairments. This study aims to simplify voice control for hearing with instant control and maintain the user's sense of navigation while the conversation is in progress.

Invasive BCIs can be directly implanted into the brain, offering high precision but involving surgical risks (Caria *et al.* 2011). Non-invasive BCIs can utilize external devices like EEG caps or headsets. These are safer and more commonly used for consumer applications (Guger *et al.* 2024). The most common non-invasive method captures electrical activity from the scalp. It's portable and relatively affordable (Alkaff *et al.* 2024). Measures brain activity by detecting changes in blood flow. It's less common but offers better spatial resolution than EEG. Measures magnetic fields produced by neural activity (Mansouri, 2023). It's less portable and more expensive but provides high spatial and temporal resolution (Araújo *et al.* 2024).A nano-enabled BCI system should have signal processing algorithms to filter noise and extract relevant features. Machine learning models should be trained to accurately interpret the user's brain signals related to volume control commands (e.g., increase, decrease, mute) (Kumar *et al.* 2024). The device should be comfortable to wear for extended periods. It should have a user-friendly interface and easy setup process. The BCI system should provide high accuracy in interpreting the user's commands. It should have a low latency to ensure real-time control of the audio system. One must ensure the BCI is compatible with your existing audio system or can be easily integrated. Evaluate the cost of the BCI system and balance it with the features and performance it offers (Liu *et al.* 2024). In this investigation novelly tried a BCI-assisted headset was developed to test the instant voice control on hearing. The performance of instant voice control with a default set of hearing levels in the conventional hearing aid was examined. This study compares the hearing performance of age-related Nano-porous Membrane Sensitivity patients wearing hearing aids with the performance of a thought-assisted voice-controlled speaker headset while listening to the TV.

2. MATERIALS AND METHODS

This study setting consists of a TV with a media player in a room with neglected environmental noise disturbance. The TV was played with a listenable volume by a normal person. The patient is then requested to tell the story or convey their understanding. The average of both known and unknown video responses was recorded for further analysis. There was no display of the hearing volume measurement. Only the patient's response was considered for evaluation. There were 3 known and 3 unknown videos per patient to justify the hearing performance. Only one patient was tested at a time. There was no interaction permitted among patients. A sample size of 20 per type of hearing assistance was estimated with a G-power of 80%, an error level of 5% and a 95% confidence interval. Statistics were taken for both groups with conventional hearing aids and for patients with a thought-assisted one-side speaker headset. The headset was equipped with a brain-computer interface for regulating hearing volume instantly through thoughts (Sargunapathi et al. 2020).

There was a 'Fixed' group with individuals of different ages and genders using hearing aids. They were prepared by explaining the testing procedure and the benefits of hearing aids while watching TV. The patients were randomly tested with different nanoporous membrane sensitivity levels. As patients used their hearing aids, they were considered to be hearing well with their hearing aids, as normal human beings. The patients were allowed to use their hearing aid on the same ear as per their comfort. The other ear was kept free for listening together.

The patients belonging to 'BCI_Navig' were trained to navigate the volume. The system navigates with the use of the key thought 'Oh my god' for reducing the volume; the key thought 'Okay' to stop navigation. The thought of 'pardon' was for increasing the volume until the patient said 'Okay'. Individuals were given practice as per their learning capacity. They were allowed to adjust the volume to their comfort zone. The headset was fixed to the patient's ear instead of the hearing aid for this investigation. Also, the patient was allowed to uncover the other ear for listening.

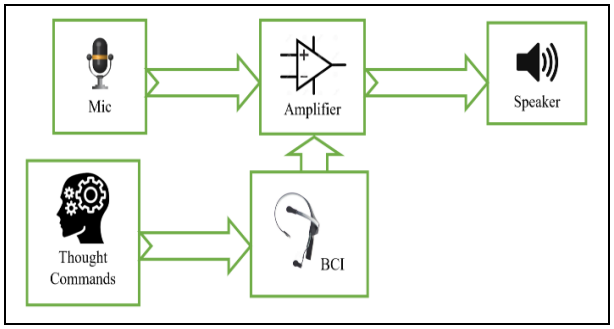


Fig. 1: Set up details of the headset

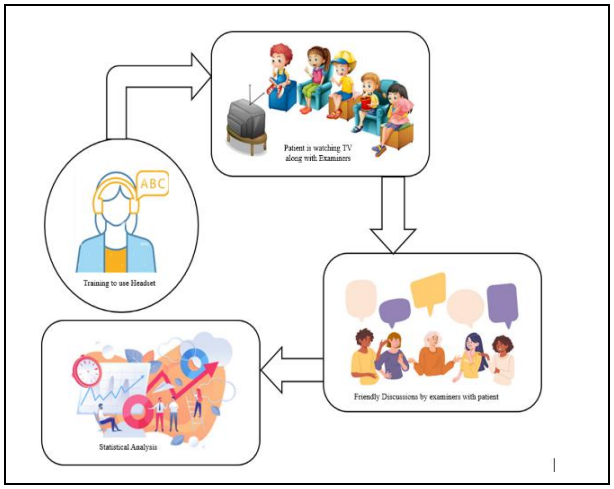


Fig. 2: Experimental setup of the examination process

The experimental setup on the headset is shown in Fig. 1. The Sony-made PHA-1A amplifier, the universal headset microphone of model SP-1167-v1.0-ME-II-3, and the 80 to 125 dB/mW headset speaker were obtained from Mercy Electronics, Vadapalani, Chennai, Tamil Nadu. The mic, which is fixed on the earplug on the headset, receives the opponent's voice and sends it to the amplifier. The amplifier modulates the volume of noise as desired by the user (the patient) based on the thought commands. Hence, instant navigation happens when the speaker is connected to the earbud, which is located behind the mic. The amplifier works in between them.

3. RESULTS AND DISCUSSION

The observations were evaluated by three therapy experts based on the response of the patient. The interaction questions were based on the content watched on TV (Fig. 2). The evaluation was based on the understanding of the conversation in the TV drama. The average of all observations was evaluated as a percentage. There were two kinds of observations: Fixed and 'BCI_Navig'. The Fixed group consisted of patients watching TV with their hearing aids. 'BCI_Navig' group comprised patients with BCI headsets to watch TV. The sample size per case (group) tested was 20 patients. It was observed that the average hearing response while watching TV improved by 18.25% with a BCI headset; *i.e.*, the average response from the same set of patients improved from 64.25% to 82.50% with use of BCI headsets (Table 1). The performance is depicted by the G graph, which is shown in Fig. 3. The graph was plotted with a 95% confidence interval. The error bars shown in the graph were plotted with the standard deviation of ±1%. The Standard Deviation of hearing responses was found to be much higher (4.88688) for patients watching TV with their own hearing aid than those who watched with a BCI headset (3.06937). Similarly, the Standard Error Mean of hearing responses for hearing aid and BCI headset users was 1.09274 and 0. 68633, respectively. Hence, it is obvious that the BCI headset decreased the Standard Deviation and Standard Error Mean of hearing responses considerably.

Table 1. Statistical analysis results

S. No.	Statistical parameters	Observations with Hearing Aid - 'Fixed' Group	Observations with BCI headset-'BCI_Navig' Group
1	Number of samples	20 patients	20 patients
2	Average hearing response (%)	64.2500%	82.5000%
3	Standard deviation of hearing responses	4.88688	3.06937
4	Standard Error Mean of hearing responses	1.09274	0. 68633

The observations were statistically analysed with an independent-samples t-test. Table 2 shows the results of Levene's test for equality of variances is hypothetical output. Any one case can be considered either "Assumed equal variances in hearing responses" or

"NOT Assumed equal variances in hearing responses." if the value of significance is less than 0.05, the Assumed equal variances in hearing responses case is to be considered in Table 3 that is, only column 3 values in Table 3, else only column 4 values in Table 3 are to be considered. From the statistical results, it is observed that both group observations are statistically and significantly different. The proposed method shows considerable improvement. This is because of the significance value of 0.015 (Table 2). As the obtained significance value is less than 0.05, both observations are considerably different and statistically significant. The two-tailed significance (0.000) (Table 3) is less than 0.05, confirming significant differences among the groups, i.e., showing significant improvement recorded with the proposed solution.

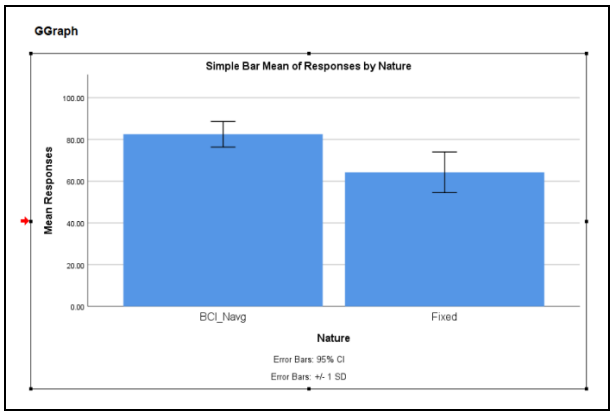


Fig. 3: Depiction of performance by G Graph

Table 2. Results of Levene's test for equality of variances

S. No.	Description of the Statistics	Assumed equal variances in hearing responses	NOT assumed as Equal variances in hearing responses
1	Value of F	6.512	-
2	Value of Significance	0.015	-

Table 3. t-Test results for equality of means for hearing response

S. No.	Description of the Statistics		Assumed equal variances in hearing responses	NOT assumed as Equal variances in hearing responses
1	Value of t		-14.143	-14.143
2	Value of df		38.000	31.972
3	Value of Sig. (2-tailed)		0.000	0.000
4	Value of mean difference		-18.25000	-18.25000
5	Value of Std. error difference		1.29040	1.29040
6	95% confidence interval of the difference	Lower Limit Value	-20.86228	-20.87855
		Upper Limit Value	-15.63772	-15.62145

A study was conducted using a randomised, repeated-measures design with 15 older adults (aged 59 to 82) with bilateral sensorineural hearing impairments who wear hearing aids. Just 13% of the participants had utilised closed captioning, whereas the majority (73%) used their hearing devices while enjoying TV on a daily basis (Gordon-Salant and Callahan, 2009). A total of 2956 residents of the Blue Mountains, west of Sydney, among the 3914 eligible individuals between the ages of 49 and 99 (mean age 67.4 years), completed a hearing study carried out between 1997 and 2003. Thirty-three percent of those who responded to the poll experienced nanoporous membrane sensitivity in their better ear. Eleven percent of the respondents had a hearing aid and 4.4% had used an assistive listening device in the previous 12 months. Of those who now possess aids, 24% have never worn them. It has been discovered that using hearing aids and assistive listening devices is linked to ageing, nano-porous membrane sensitivity, and self-perceived hearing impairment (Hartley *et al.* 2010). Two-thirds of hard-of-hearing viewers over the age of 51 who were granted access to the teletext subtitle service said that subtitles helped them comprehend television shows (Dülger and Dülger, 2022). The viewers who are hard of hearing reported using subtitles the most out of all those who had teletext. About 13% of hearing-impaired adults over the age of 51 reported using subtitles for every program they watched, while another 26% of those over 55 reported doing so on a frequent basis for certain programs (Sancho-Aldridge and Davis, 1993). 180 elderly people with nanoporous membrane sensitivity participated in a prospective study that included neuropsychologic, quality-of-life and audiologic assessments. The participants were divided into four groups and given four treatment conditions: one that involved no amplification at all and one that involved three different forms of amplification (conventional hearing aid, assistive listening device, and combination of the two systems). Every individual agreed to take part in research comparing various amplification devices in exchange for payment. There was a significant preference for the traditional hearing aid in daily usage by the older users who were often unwilling to put up with the challenges that come with using remote microphone devices (Jerger *et al.* 1996). In the Chicago metropolitan region, research was conducted to compare adolescent television viewers with normal hearing versus those with hearing impairments. In the first comparison, the duration of time spent watching television was examined. For all adolescent television watchers, the average weekly time spent watching television was 20.43 hours; for hard-of-hearing viewers, it was 30.98 hours; and for deaf respondents, it was 36.75 hours. The preference of viewers for different programmes by title was the second component of television watching that was studied. The findings showed that the three categories of television viewers—those with normal hearing, those who are hard of hearing, and those who are deaf—each had distinct preferences for the shows they watch. The final area under investigation was limited to the respondents with hearing impairment (Sendelbaugh, 1978).

The limitation of this research is that, though headset use supports good hearing, continuous headset

use is not acceptable to the user. The social acceptance of different kinds of wear is a time-consuming process, but this concept may include instant control of the hearing aid, which is very useful to the user to enjoy TV shows. Training people near 70 has some difficulties and consumes more time.

4. CONCLUSION

The present investigation demonstrates the potential of nanotechnology-enabled sensor systems for improving signal detection and sensitivity in advanced sensing applications. Twenty different nanomaterial substrates, fabricated within the nanoscale range of approximately 50–70 nm, were evaluated using different baseline and test signal conditions. The comparative assessment indicated that the nano-oriented BCI-assisted sensor system provided improved signal reception and real-time monitoring capability compared with the conventional acoustic nano-substrate approach. The observed 18.25% enhancement in signal perception and decoding, together with the statistically significant improvement ($p < 0.001$), indicates that the integration of nanoscale sensing materials with intelligent signal-processing approaches may provide an effective strategy for compensating for sensitivity losses in sensor systems.

From an environmental nanotechnology perspective, the findings highlight the broader potential of engineered nanomaterials as sensitive transduction platforms for the detection and monitoring of weak or variable signals. The high surface-to-volume ratio and tunable physicochemical properties of nanostructured materials can facilitate the development of compact, responsive, and adaptable sensing systems with potential applications in environmental monitoring, pollutant detection, chemical sensing, and real-time assessment of environmental parameters. The incorporation of intelligent sensitivity-control mechanisms may further improve the reliability and adaptability of such nanoscale sensor platforms under changing operating conditions.

Nevertheless, the study has certain limitations, particularly the relatively limited number of nanomaterial substrates evaluated and the need for systematic investigation of material composition, morphology, surface characteristics, signal-to-noise ratio, long-term stability, and environmental operating conditions. Future research should therefore focus on optimizing nanomaterial architecture and surface functionality, establishing structure–property–sensing relationships, and evaluating the performance of these systems using environmentally relevant chemical and biological analytes. Integration with low-power electronics, wireless monitoring, and artificial-intelligence-assisted signal analysis could further enhance their practical applicability.

Overall, this study provides preliminary evidence that the integration of engineered nanomaterials with intelligent sensing and signal-processing technologies can contribute to the development of highly sensitive and adaptive nanosensor platforms. Such advances may support the development of next-generation environmental sensing technologies for rapid, selective, and real-time monitoring of contaminants and environmental changes.

FUNDING

There is no funding source.

CONFLICT OF INTEREST

The authors declared no conflict of interest in this manuscript regarding publication.

COPYRIGHT

This article is an open-access article distributed under the terms and conditions of the Creative Commons Attribution (CC BY) license (http://creativecommons.org/licenses/by/4.0/).

REFERENCES

Acuña, K., Sapahia, R., Jiménez, I. N., Antonietti, M., Anzola, I., Cruz, M. and DeBuc, D. C., (2024). Functional Near-Infrared Spectrometry as a Useful Diagnostic Tool for Understanding the Visual System: A Review, *J. Clin. Med.*, 13(1), 282 (2024). https://doi.org/10.3390/jcm13010282

Ahmadian, P., Cagnoni, S. and Ascari, L., How capable is non-invasive EEG data of predicting the next movement? A mini review, *Front. hum. neurosci.*, 7, 124 (2013). https://doi.org/10.3389/fnhum.2013.00124

Alkaff, Z. A., Malim, N. H. A. H., Sumari, P. and Abdullah, J. M., Applications of Brain Computer Interface in Present Healthcare Setting, (2024). https://doi.org/10.5772/intechopen.112353

Araújo, J., Simons, B. D. and Goswami, U., Remediating phonological deficits in dyslexia with brain-computer interfaces, *In Brain-Computer Interface Research: A State-of-the-Art Summary*, 11, 13-19 (2024). Cham: Springer Nature Switzerland. https://doi.org/10.1007/978-3-031-49457-4_2

Belkacem, A. N., Nishio, S., Suzuki, T., Ishiguro, H. and Hirata, M., Neuromagnetic decoding of simultaneous bilateral hand movements for multidimensional brain–machine interfaces, *IEEE Trans. Neural Syst. Rehabil. Eng.*, 26(6), 1301-1310 (2018). https://doi.org/10.1109/TNSRE.2018.2837003

Belkacem, A. N., Saetia, S., Zintus-Art, K., Shin, D., Kambara, H., Yoshimura, N. and Koike, Y., Real-Time Control of a Video Game Using Eye Movements and Two Temporal EEG Sensors, *Comput.*

Intell. Neurosci., 2015(1), 653639 (2015). https://doi.org/10.1155/2015/653639

Calhoun, V. D., Amin, M. F., Hjelm, D., Damaraju, E. and Plis, S. M., A deep-learning approach to translate between brain structure and functional connectivity, *IEEE Int. Trans. Acoust., Speech, Signal. Pro. (ICASSP)*, 6155-6159 (2017). https://doi.org/10.1109/ICASSP.2017.7953339

Caria, A., Weber, C., Brötz, D., Ramos, A., Ticini, L. F., Gharabaghi, A. and Birbaumer, N., Chronic stroke recovery after combined BCI training and physiotherapy: a case report, *Psychophysiology*, 48(4), 578-582 (2011). https://doi.org/10.1111/j.1469-8986.2010.01117.x

Hartley, D., Rochtchina, E., Newall, P., Golding, M. and Mitchell, P., Use of hearing aids and assistive listening devices in an older Australian population, *J Am Acad Audiol.*, 21(10), 642-653 (2010). https://doi.org/10.3766/jaaa.21.10.4.

Falk, T. H., Guger, C. and Volosyak, I., Brain–computer interfaces: recent advances, challenges, and future directions, *Handbook of Hum. Mach. Syst.*, 11-22 (2023). https://doi.org/10.1002/9781119863663.ch2

Gordon-Salant, S. and Callahan, J. S., The benefits of hearing aids and closed captioning for television viewing by older adults with hearing loss, *Ear and Hear.*, 30(4), 458-465 (2009). https://doi.org/10.1097/AUD.0b013e3181a26ef4

Guger, C., Ince, N. F., Korostenskaja, M. and Allison, B. Z., Brain-Computer Interface Research: A State-of-the-Art Summary 11, *In Brain-Computer Interface Research: A State-of-the-Art Summary*, 11, 1-11 (2024). Cham: Springer Nature Switzerland. https://doi.org/10.1007/978-3-031-49457-4_1

Guger, C., Rezvani, S., Ince, N. F., Korostenskaja, M. and Allison, B. Z., A Summary of the 2022 BCI Award with Discussion of BCI Trends, *In Brain-Computer Interface Research: A State-of-the-Art Summary*, 11, 141-148 (2024). https://doi.org/10.1007/978-3-031-49457-4_13.

Huo, C., Xu, G., Xie, H., Chen, T., Shao, G., Wang, J. and Li, Z., Functional near-infrared spectroscopy in non-invasive neuromodulation, *Neural Regen. Res.*, 19(7), 1517-1522 (2024). https://doi.org/10.4103/1673-5374.387970

Jerger, J., Chmiel, R., Florin, E., Pirozzolo, F. and Wilson, N., Comparison of conventional amplification and an assistive listening device in elderly persons. *Ear and hear.*, 17(6), 490-504 (1996).

Lal, T., Hinterberger, T., Widman, G., Schröder, M., Hill, N., Rosenstiel, W. and Schölkopf, B., Methods towards invasive human brain computer interfaces, *Adv. Neural Inf. Process. Syst.*, 17 (2004).

Lekova, A. K., Tsvetkova, P. and Andreeva, A., Enhancing Brain Health and Cognitive Development Through Sensorimotor Play in Virtual Reality: Uncovering the Neural Correlates, *Int. J. Games Soc. Impact*, 2(1), 46-70 (2024). https://www.doi.org/10.24140/ijgsi.v2.n1.03

Liu, S., Wang, L. and Gao, R. X., Cognitive neuroscience and robotics: Advancements and future research directions, *Robot. Comput. Integr. Manuf.*, 85, 102610 (2024). https://doi.org/10.1016/j.rcim.2023.102610.

Maiseli, B., Abdalla, A. T., Massawe, L. V., Mbise, M., Mkocha, K., Nassor, N. A. and Kimambo, S., Brain–computer interface: trend, challenges, and threats, *Brain Inform.*, 10(1), 20 (2023). https://doi.org/10.1186/s40708-023-00199-3

McFarland, D. J. and Wolpaw, J. R., Brain-computer interfaces for communication and control, *Com. ACM.*, 54(5), 60-66 (2011). https://doi.org/10.1145/1941487.1941506

Munavalli, J. R., Sankpal, P. R., Sumathi, A. Oli, J. M., Introduction to Brain–Computer Interface: Applications and Challenges, *Brain-Computer Interface: Using Deep Learning Applications*, 1-24 (2023). https://doi.org/10.1002/9781119857655.ch1

Nielsen., The total audience report Q1, 2017, The Nielsen Company (US), LLC., New York, NY. (2017).

Okorokova, E. V., Sobinov, A. R., Downey, J. E., He, Q., van Driesche, A., Satzer, D. and Bensmaia, S. J., May the Force Be with You: Biomimetic Grasp Force Decoding for Brain Controlled Bionic Hands, *In Brain-Computer Interface Research: A State-of-the-Art Summary* 11, 109-121 (2024). https://doi.org/10.1007/978-3-031-49457-4_11

Romine, C. B. and Reynolds, C. R., Sequential memory: a developmental perspective on its relation to frontal lobe functioning, *Neuropsychol. Rev.*, 14, 43-64 (2004). https://doi.org/10.1023/B:NERV.0000026648.94811.32

Sancho-Aldridge, J. and Davis, A., The impact of hearing impairment on television viewing in the UK, *Br. J. Audiol.*, 27(3), 163-173 (1993). https://doi.org/10.3109/03005369309076690

Schalk, G., McFarland, D. J., Hinterberger, T., Birbaumer, N. and Wolpaw, J. R., BCI2000: a general-purpose brain-computer interface (BCI) system. *IEEE Trans. Biomed. Eng.*, 51(6), 1034-1043 (2004). https://doi.org/10.1109/TBME.2004.827072

Schalk, G. and Allison, B. Z., Noninvasive brain–computer interfaces, *In Neuromodulation*, 357-377 (2018). https://doi.org/10.1016/B978-0-12-805353-9.00026-7

Sendelbaugh, J. W., Television viewing habits of hearing-impaired teenagers in the Chicago metropolitan area, *Am. Ann. Deaf*, 536-541 (1978). http://www.jstor.org/stable/44399792

Tao, Q., Chao, H., Fang, D. and Dou, D., Progress in neurorehabilitation research and the support by the National Natural Science Foundation of China from 2010 to 2022, *Neural Regen. Res.*, 19(1), 226-232 (2024). https://doi.org/10.4103/1673-5374.375342

Woodman, G. F., A brief introduction to the use of event-related potentials in studies of perception and attention, *Atten. Percept. Psychophys.*, 72, 2031-2046 (2010). https://doi.org/10.3758/BF03196680

Kumar, Y., Kumar, J. and Sheoran, P., Integration of cloud computing in BCI: A reviewBiomed. Signal

Process. Control., 87, 105548 (2024). https://doi.org/10.1016/j.bspc.2023.105548

Mansouri, S., Application of Neural Networks in the Medical Field, *Journal of Wireless Mobile Networks, Ubiquitous Computing, and Dependable Applications*, 14(1), 69-81 (2023). https://doi.org/10.58346/JOWUA.2023.I1.006

Ilić, P., Nešković Markić, D. and Stojanović Bjelić, L., Measuring and Mapping Noise Pollution in the City of Banja LUKA, *Archives for Technical Sciences*, 1(18), 89–96 (2018). https://doi.org/10.7251/afts.2018.1018.089I

Sargunapathi, R., Vinayagamoorthy, P., Sumathi, P. and Sirajunissa Begum, S., Mapping of Scientific Articles on Brain Tumors: A Scientometric Study, *Indian Journal of Information Sources and Services*, 10(2), 26–34 (2020). https://doi.org/10.51983/ijiss.2020.10.2.490

Dülger, G. and Dülger, B., Antibacterial Activity of Stachys sylvatica Against Some Human Eye Pathogens, *Natural and Engineering Sciences*, 7(2), 131-135 (2022). https://doi.org/10.28978/nesciences.1159224

Kadhim, A. A., Mohammed, S. J. and Al-Gayem, Q., Digital Video Broadcasting T2 Lite Performance Evaluation Based on Rotated Constellation Rates, Journal of Internet Services and Information Security, 13(3), 127-137 (2023). https://doi.org/10.58346/JISIS.2023.I4.009